

Evaluation of a New ELISA for Detection of *Blastomyces dermatitidis* Antigen in Urine

Michael Scott Bennett^a, Timothy Crane^b, Andre Albert^b, and Marc Roger Couturier^{a,c}

^aAssociated Regional and University Pathologists, Inc., Salt Lake City, UT

^cGotham Biotechnology, New Gloucester, ME

^cDepartment of Pathology, University of Utah, Salt Lake City, UT

500 Chipeta Way
Salt Lake City, UT 84108-5207
Michael.Bennett@aruplab.com

Sunday-CPHM-887

Revised Abstract

Background

Blastomyces dermatitidis is the causative agent for blastomycosis, an endemic fungal infection prevalent in the Ohio and Mississippi River Valleys, Great Lakes region, and the Southeastern United States. It causes acute and chronic pneumonia, as well as disseminated extrapulmonary disease. Currently, the only commercially available testing for Blastomyces antigen is through Mira Vista Laboratories. Our laboratory has performed the first evaluation of a novel ELISA test, the Gotham Biotechnology Blastomycosis Urinary Antigen Detection ELISA, as an alternative commercially available test.

Methods

Urine samples previously tested using the Mira Vista Blastomyces ELISA were used as a comparator for accuracy. Dilutions of high positive urine samples in urine matrix were performed to test linearity. Both within run and between run reproducibility was tested on patient urine samples. Samples were kept refrigerated at several intervals up to 30 days, and up to 4 freeze thaw cycles were tested to determine analyte stability. Antigen from several microorganisms were tested to determine analytical specificity.

Results

Compared to Mira Vista results, the Gotham ELISA showed 93.3% (28/30) positive agreement and 100% (30/30) negative agreement. The assay was found to be quantitative and linear within the range of the calibrators, and had low intra-assay and inter-assay variability. Urine samples were found to be stable for at least 30 days refrigerated, and at least 4 freeze thaw cycles. Cross reactivity was observed with *Histoplasma capsulatum* and *Coccidioides immitis*.

Methods

Patients and Reference Subjects: De-identified human urine samples, tested previously at Mira Vista Laboratories for the presence of *Blastomyces dermatitidis* antigen, were tested by the Gotham Blastomyces ELISA (30 positive and 30 negative). Of the positive urine sample, 21 were from patients for which testing at ARUP had confirmed *Blastomyces dermatitidis* infection by other methods (DNA probe, MALDI-TOF, and/or PCR), and the remainder were from patients that did not receive this additional testing. Reference urine samples were obtained at ARUP from 20 healthy subjects who had no previous history of blastomycosis, histoplasmosis, coccidioidomycosis, or paracoccidioidomycosis, or who had lived in areas endemic for these diseases.

Calibrators and Controls: *Blastomyces dermatitidis* antigen used for calibrators and controls was derived by purification from a *Blastomyces dermatitidis* human-derived isolate as previously described (1). While antigen was provided in units of ng/mL, as there is no official W.H.O. defined *Blastomyces* antigen, levels of antigen described here are reported in non-specific EIA/mL units, with 1 ng/mL of supplied antigen being approximately equivalent to 1 EIA/mL. Calibrators and controls in synthetic urine were prepared at 20, 10, 5, 2.5, and 1.25 EIA/mL for calibrators, and 4 EIA/mL for the positive control. Samples >20 EIA/mL were tested at a 1:10 dilution in 1X wash buffer.

ELISA conditions: Calibrators, controls, and samples were loaded into a single well each of the 96 well plate, and incubated for 1 hour with shaking at room temperature. Following sample incubation, samples were washed using an automated plate washer, incubated with detector antibody conjugated to HRP, incubated for 30 minutes with shaking at room temperature, washed, and developed for 10 minutes at room temperature with the addition of Tetramethylbenzidine (TMB). After TMB incubation, Stop Solution (1N HCl) was added, and the plate was read at OD 450 nm, with subtraction of OD 650 nm.

Samples for Cross-reactivity: Cultures of type strains of *Candida albicans*, *Coccidioides immitis*, *Sporothrix schenckii*, *Talaromyces marneffeii*, and *Cryptococcus neoformans* were incubated for up to 1 week in BHI media at 37°C until a turbid suspension was visible, followed by filtration of supernatant twice through a 0.2 micron filter, and tested at a 1:10 dilution in negative human urine. Urine samples that tested positive for antigen from *Legionella pneumophila* and *Streptococcus pneumoniae* were also tested. Positive control material from an Aspergillus EIA (Platelia, Biorad) was tested 1:10 in urine, and positive control material from a *Histoplasma capsulatum* ELISA under development was spiked at 5 EIA/mL in urine.

Limit of Detection (LoD): The LoD was determined by testing 20 negative reference urine samples and 8 replicates of negative control (synthetic urine). The LoD was calculated using the negative urine average OD plus 10 standard deviations (2). This OD value was 1.27 times the negative control OD. In subsequent experiments, OD values 1.27 times or greater than the negative control were determined to be positive.

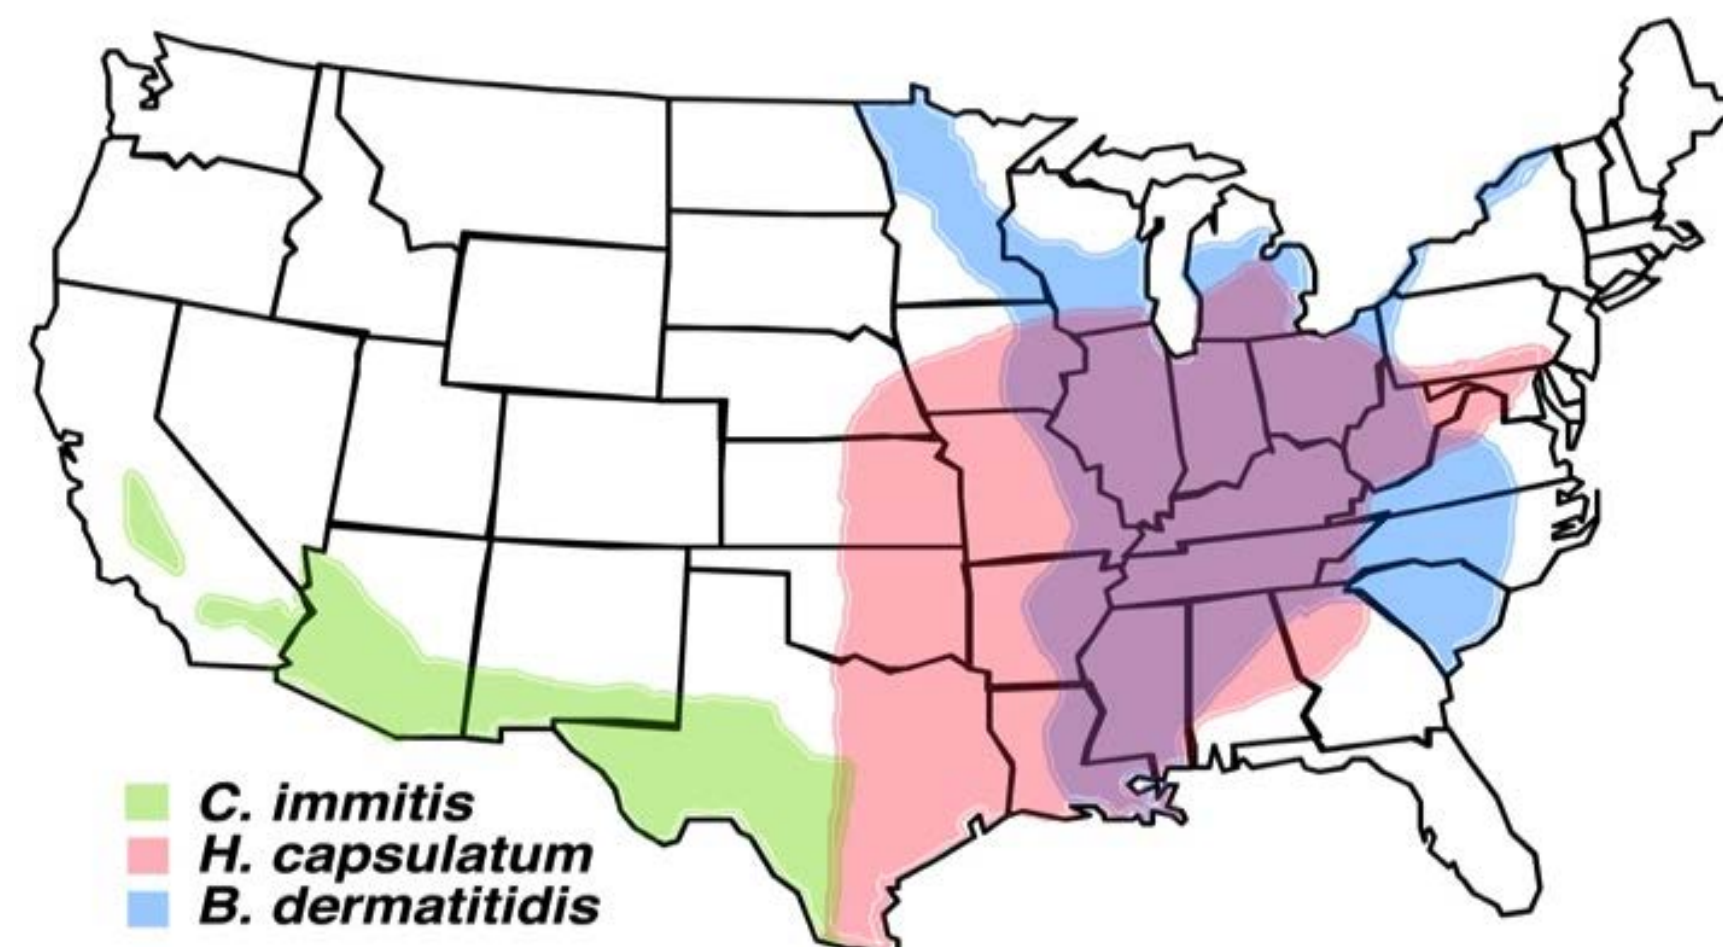


Figure 1: Regions in the U.S. endemic for *Coccidioides immitis*, *Histoplasma capsulatum*, and *Blastomyces dermatitidis*

Infectious Diseases: Blastomyces dermatitidis, by Carol Kauffman
<https://www.infectiousdiseaseadvisor.com/home/decision-support-in-medicine/infectious-diseases/blastomyces-dermatitidis/>

		Gotham			
		Positive	Negative	Total	% Agreement
Mira Vista	Positive	28	2	30	93.3%
	Negative	0	30	30	100.0%

Table 1: Overall agreement between the Gotham and Mira Vista Blastomyces ELISAs. Concordant results are highlighted in green, and discordant results are highlighted in yellow.

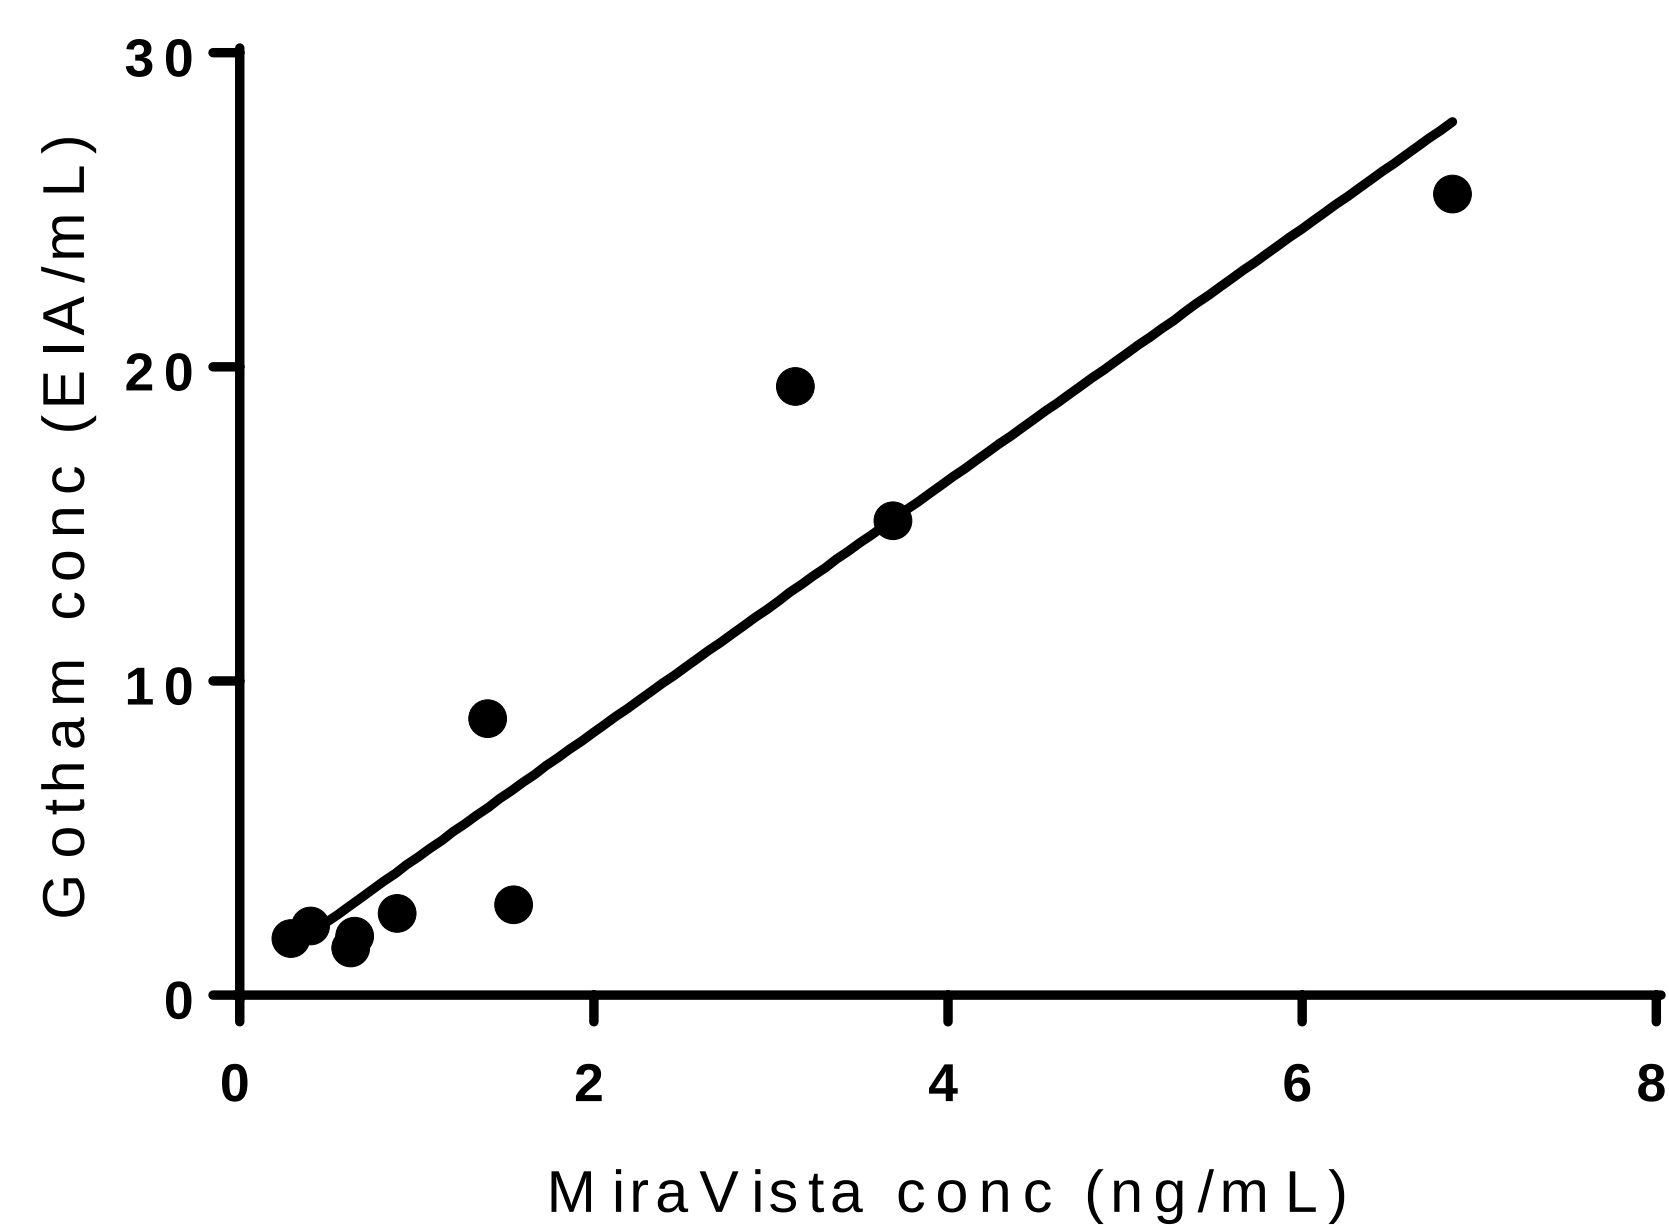


Figure 2: Urine samples tested by both Mira Vista and Gotham that were within the quantifiable range for both assays

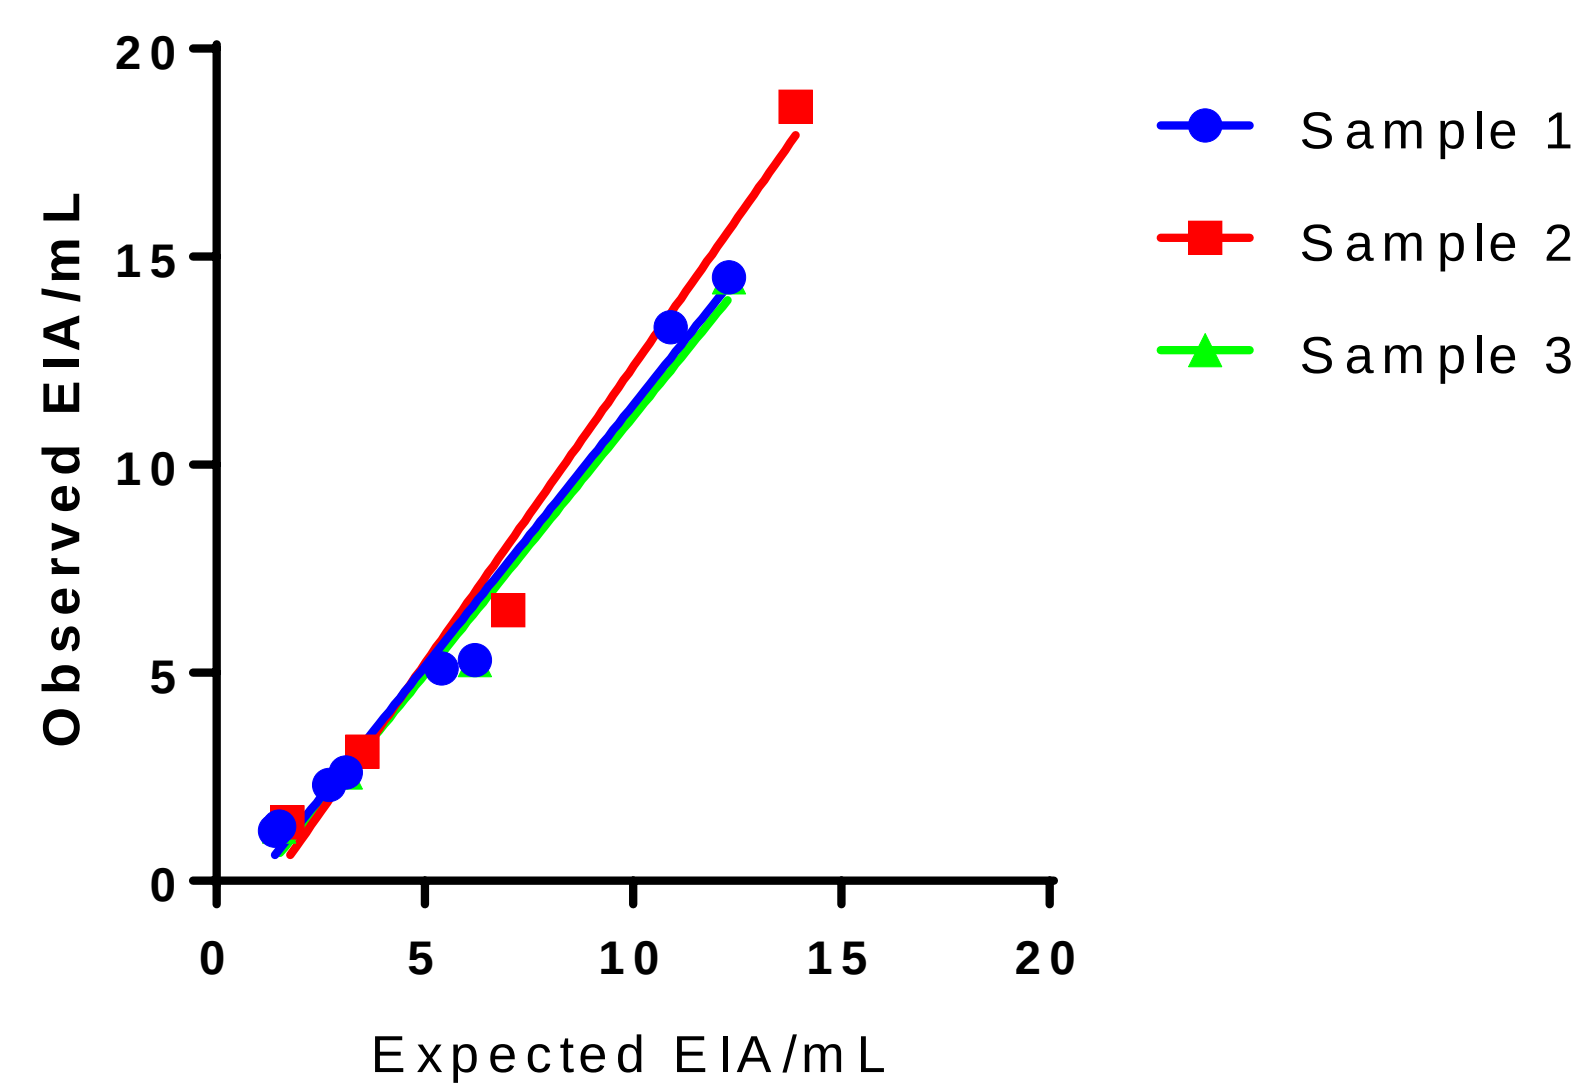


Figure 3: Linearity of three *Blastomyces* positive urine specimens, serially diluted two-fold in *Blastomyces* negative urine.

Results

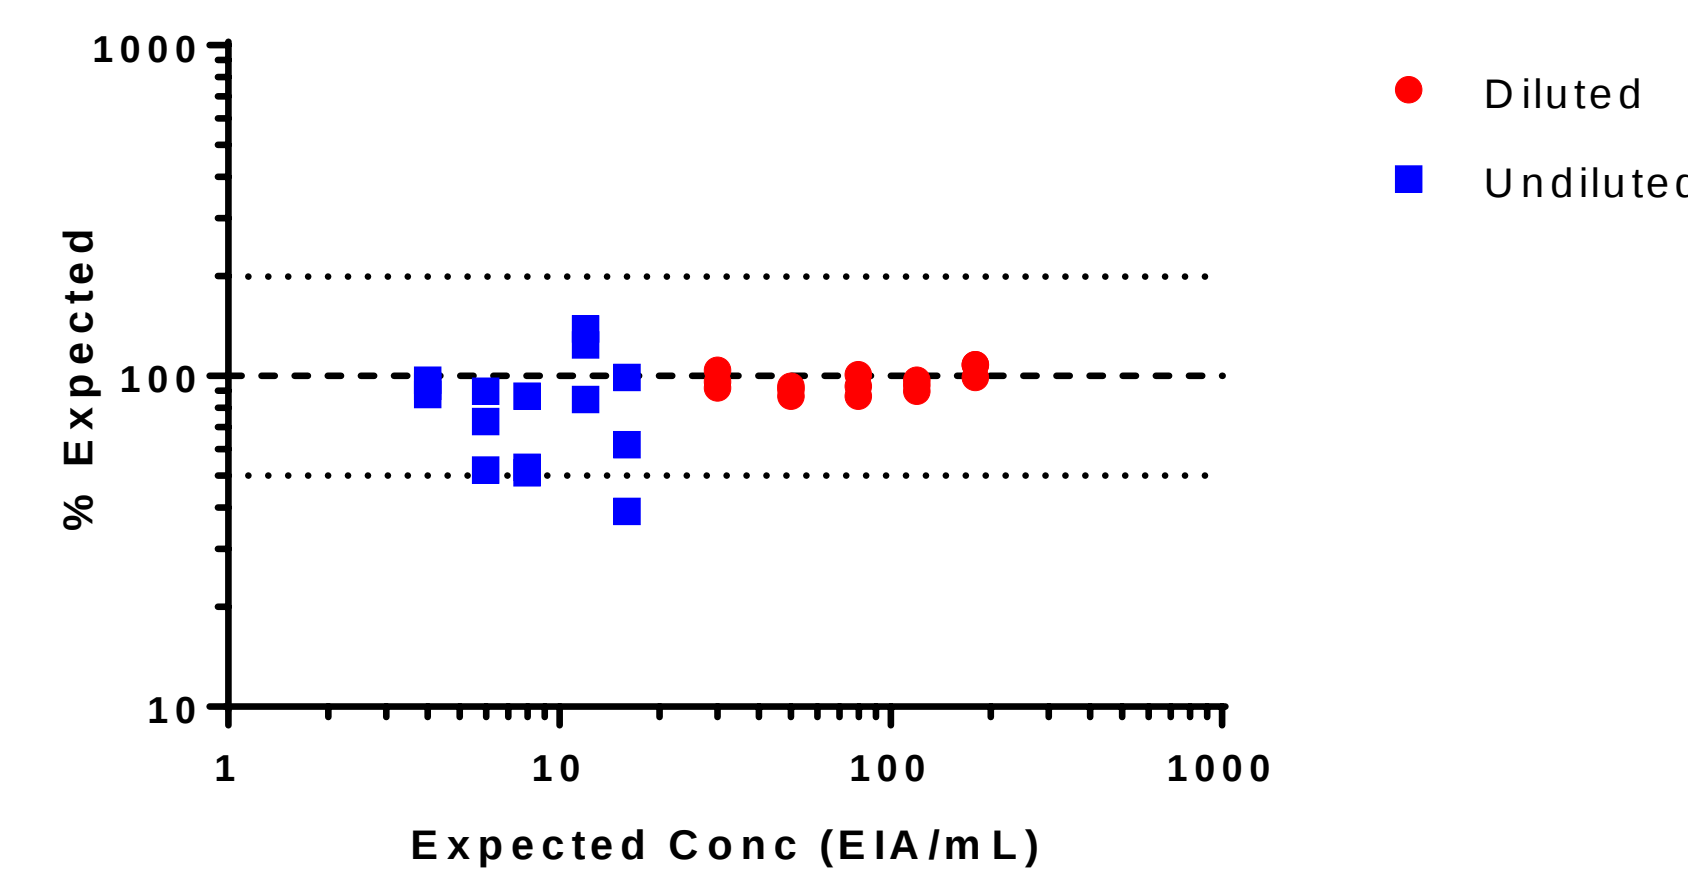


Figure 4: Recovery of *Blastomyces* antigen spiked at known concentrations into unique *Blastomyces*-negative urine samples. Red indicates samples urine sample that were diluted 1:10 in wash buffer, while blue samples were undiluted. Light dashed lines represent values 2 fold higher or lower than expected.

Organism	Preparation	Neg ctrl OD	Sample OD	EIA/mL	Result
<i>Histoplasma capsulatum</i>	5 ng/mL in urine	0.125	1.297	10.271956	Detected
<i>Coccidioides immitis</i>	1:10 culture supernatant in urine	0.125	3.266	>20	Detected
<i>Cryptococcus neoformans</i>	pos control from crypto EIA, 1:10 in urine	0.121	0.116		Not Detected
<i>Cryptococcus neoformans</i>	pos control from crypto LFA, 1:10 in urine	0.121	0.113		Not Detected
<i>Cryptococcus neoformans</i>	1:10 culture supernatant in urine	0.121	0.112		Not Detected
<i>Aspergillus</i> spp.	Pos control from Platelia assay	0.125	0.117		Not Detected
<i>Candida albicans</i>	1:10 culture supernatant in urine	0.125	0.115		Not Detected
<i>Legionella pneumophila</i>	positive urine sample	0.125	0.116		Not Detected
<i>Sporothrix schenckii</i>	1:10 culture supernatant in urine	0.125	0.115		Not Detected
<i>Streptococcus pneumoniae</i>	positive urine sample	0.125	0.130		Not Detected
<i>Talaromyces (Penicillium) marneffeii</i>	1:10 culture supernatant in urine	0.125	0.117		Not Detected

Table 2: Cross-reactivity of Gotham Blastomyces ELISA with antigen preparations from multiple organisms. Samples that showed cross-reactivity are highlighted in yellow.

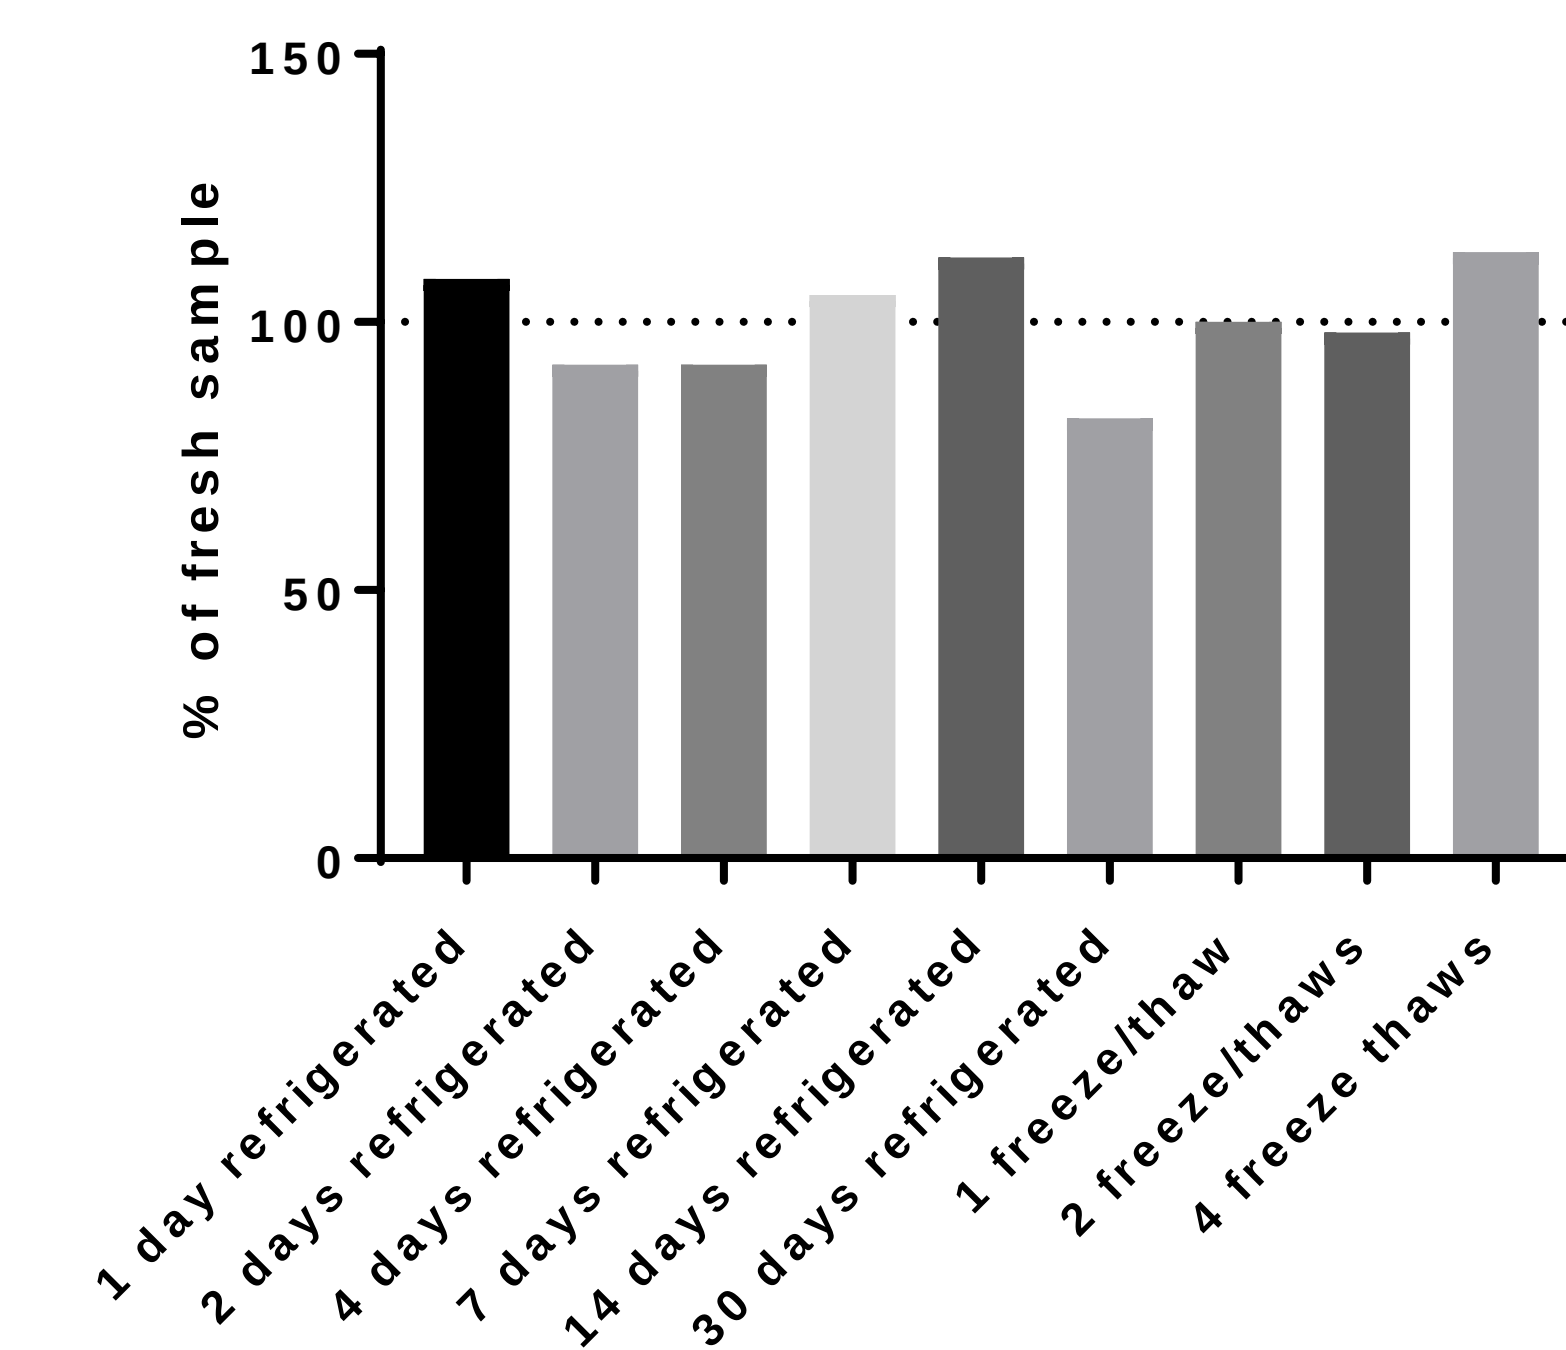


Figure 5: Stability of Blastomyces positive urine samples. Several aliquots of a single sample were frozen at -80°C, and thawed and refrigerated at multiple time points prior to testing. The results were compared to a sample thawed on the day of testing (fresh sample). Multiple freeze/thaw cycles were also tested during the same experiment.

Conclusions

- The Gotham Blastomyces ELISA shows good agreement (93% positive agreement, 100% negative agreement) with the Mira Vista Blastomyces ELISA
- The assay is linear over the range of custom calibrators, and shows good recovery for spiked urine samples
- The assay shows cross reactivity with *Histoplasma capsulatum* and *Coccidioides immitis*, but not other tested fungal antigens
- Urine samples are stable for at least 30 days refrigerated, and at least 4 freeze/thaw cycles.
- The Gotham Blastomyces ELISA shows promise for providing additional testing modalities for blastomycosis

References

- Boyd AR, Vandyke JL, Scalapone GM. 2013. Blastomyces dermatitidis Yeast Lysate Antigen Combinations: Antibody Detection in Dogs with Blastomycosis. Vet Med Int **2013**:940126.
- Andreasson U, Perret-Liaudet A, van Waalwijk van Doorn LJ, Blennow K, Chiasserini D, Engelborghs S, Fladby T, Genc S, Kruse N, Kuiperij HB, Kulic L, Lewczuk P, Mollenhauer B, Mroczko B, Parnetti L, Vanmechelen E, Verbeek MM, Winblad B, Zetterberg H, Koel-Simmelink M, Teunissen CE. 2015. A Practical Guide to Immunoassay Method Validation. Front Neurol **6**:179.